


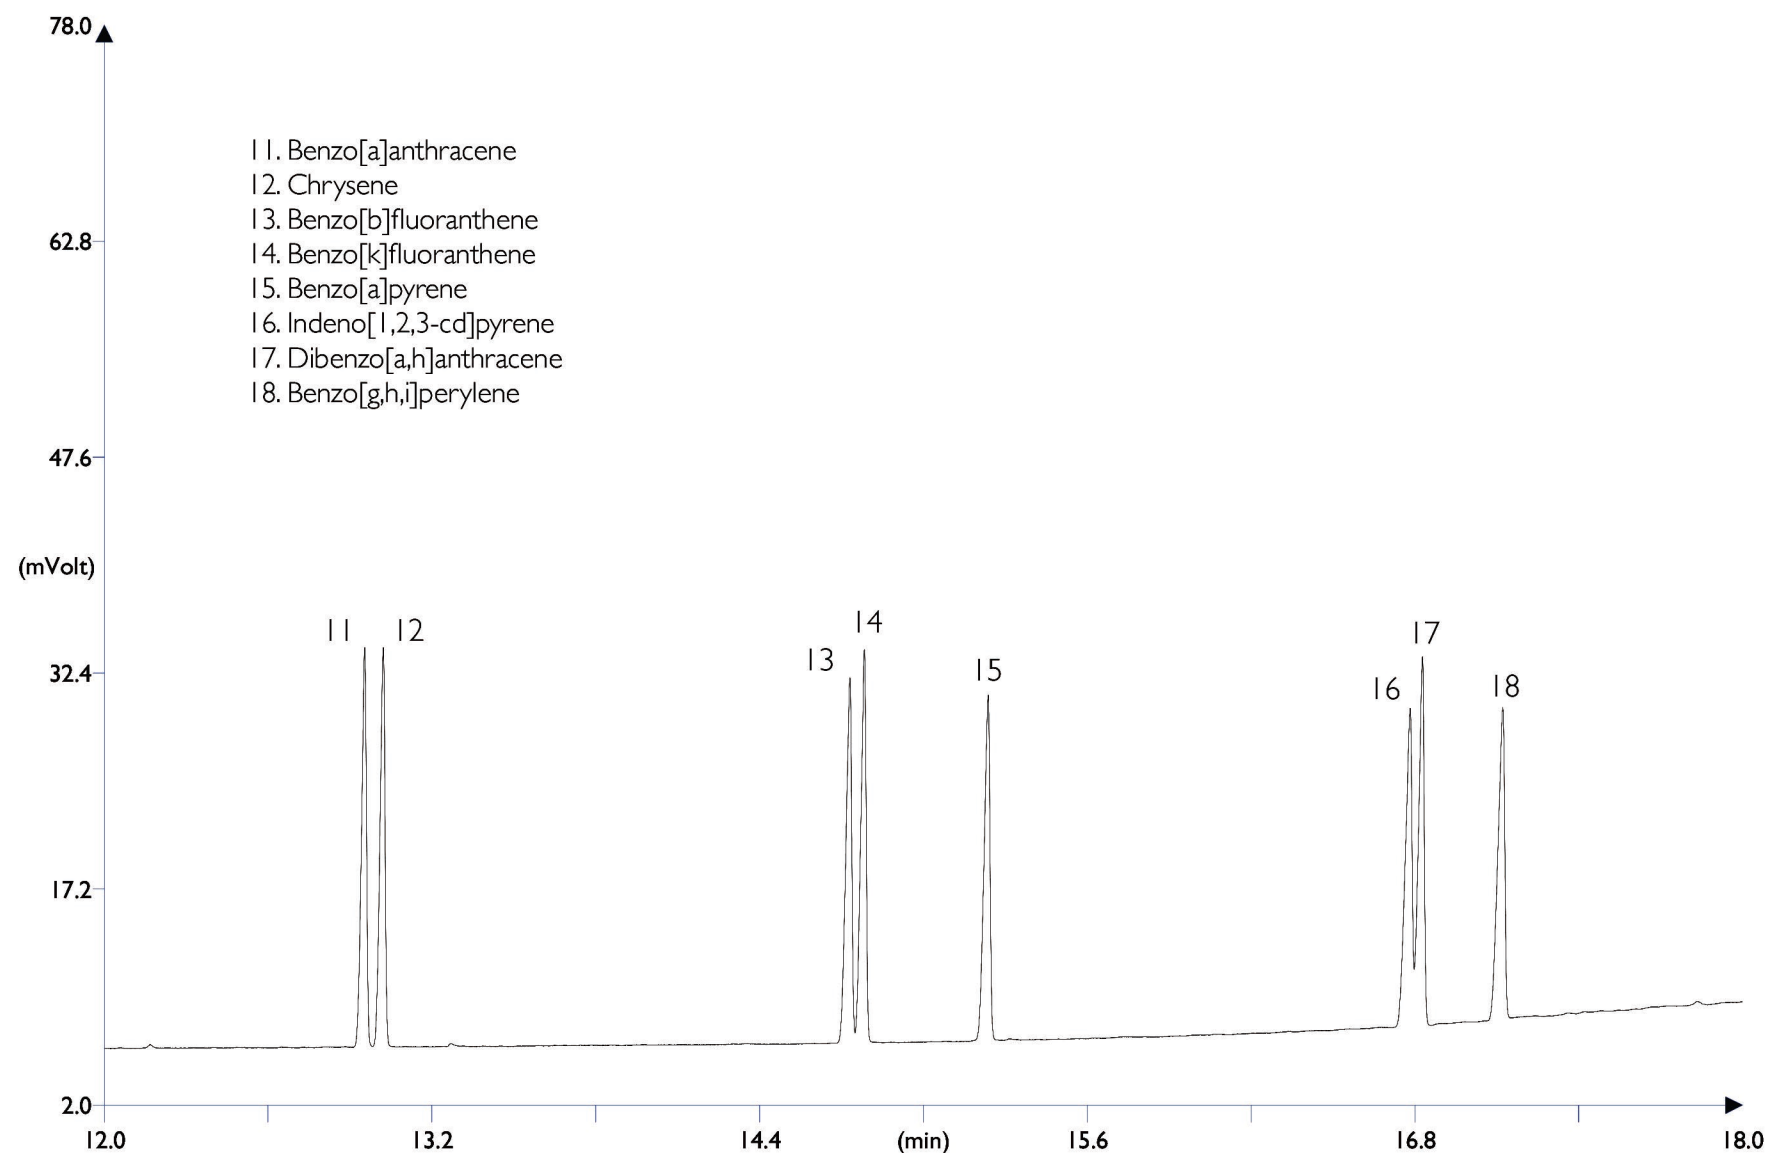

Column: **MEGA-5 MS Xil** - 0.15mm, 0.10µm, 30m

Catalog Code: MS-5XIL-015-010-30

条件:

进样口: 分流 230°C, 200mL/min 分流比, 0.2µL 进样量

检测器: FID 330°C

柱温箱程序: 90°C-300°C, 0.5°C/min

载气: 氢气, 240kPa

Sample:

8270 Calibration Mix #5, Revised 2000µg/mL in
Methylene Chloride.

EPA method 610, 8100, 8270

GO BACK
TO THE ENTIRE
CHROMATOGRAM

