


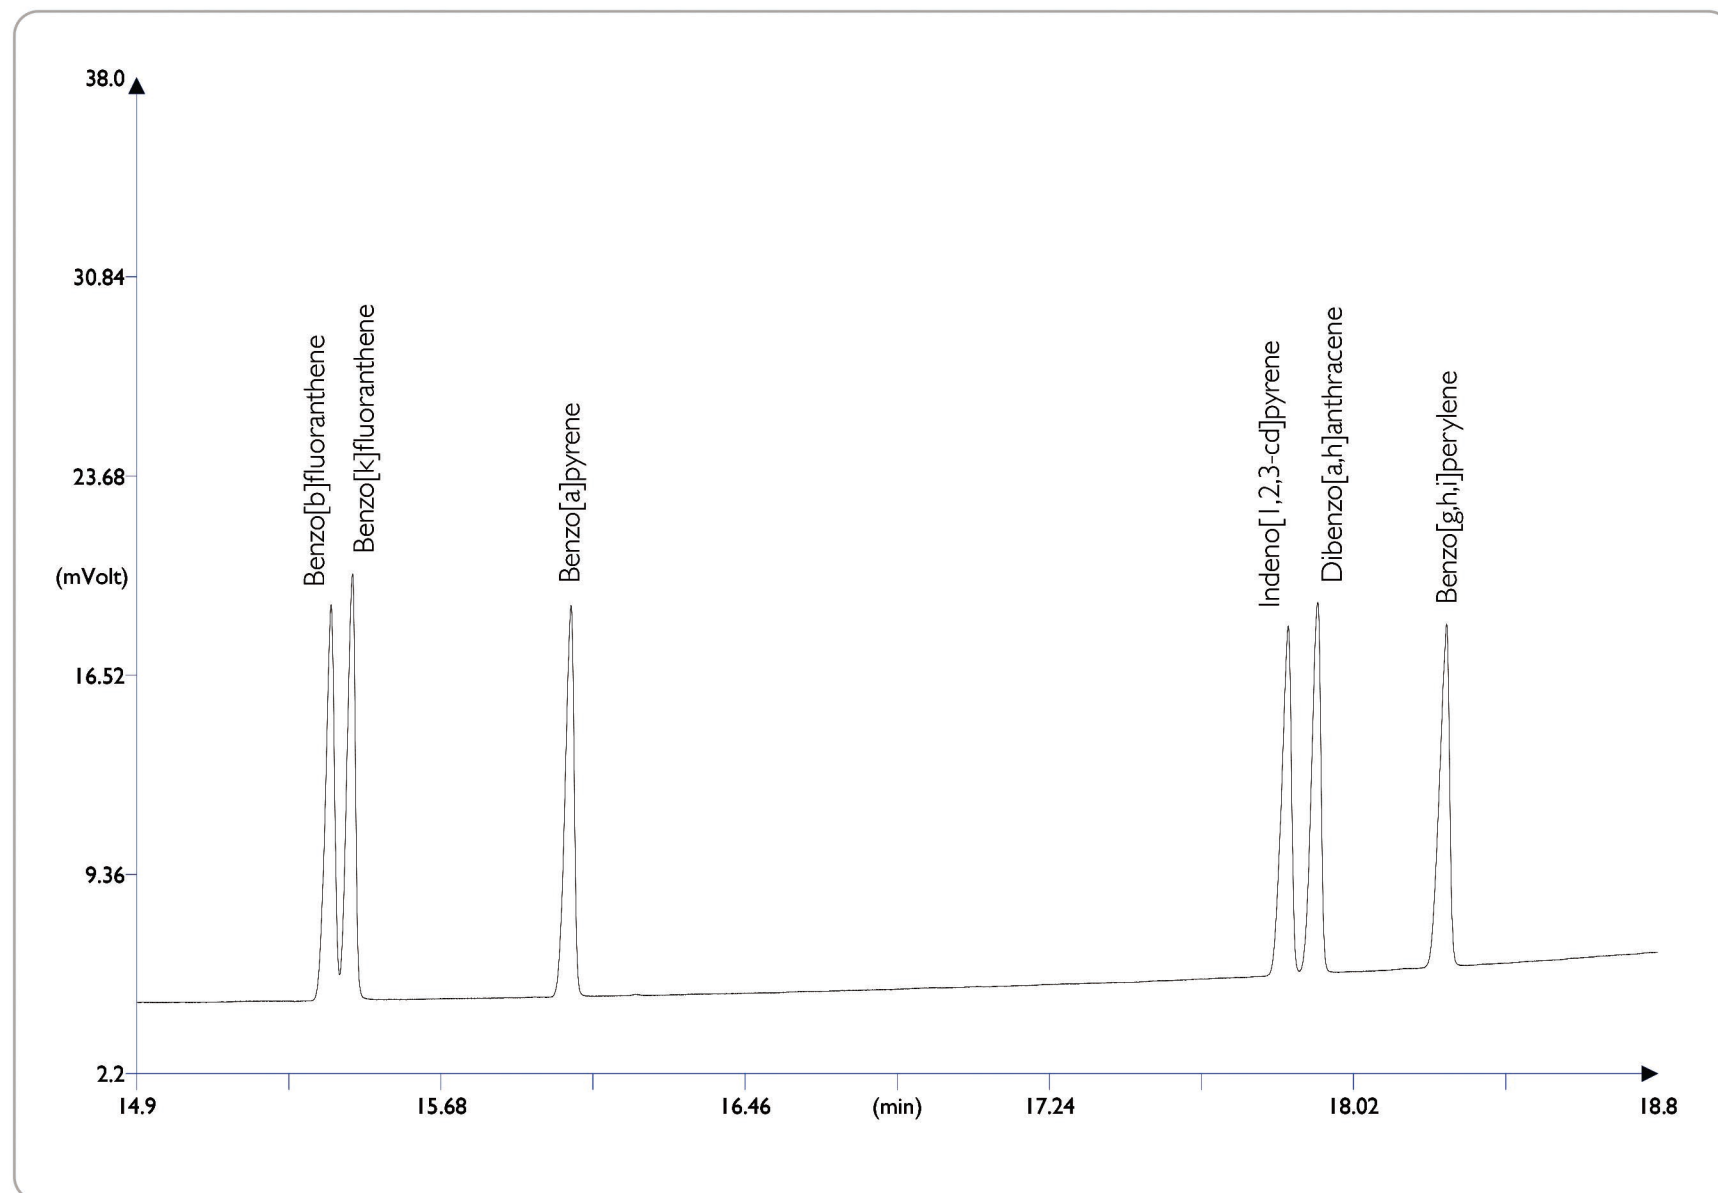

Column: **MEGA-PAH - 0.15mm, 0.15 μ m, 15m**

Catalog Code: C-PAH-015-015-15

条件:

进样口: 分流 230 $^{\circ}$ C, 300mL/min分流比, 0.2 μ L进样量

检测器: FID 330 $^{\circ}$ C

柱温箱程序: 90 $^{\circ}$ C-340 $^{\circ}$ C, 12 $^{\circ}$ C/min

载气: 氢气, 170kPa

Sample:

8270 Calibration Mix #5, Revised 2000 μ g/mL in
Methylene Chloride.

EPA method 610, 8100, 8270

GO BACK
TO THE ENTIRE
CHROMATOGRAM

