


Column: **MEGA-PS264 - 0.32mm, 5.00 μ m, 15m**

Catalog Code: C-PS264-032-500-15

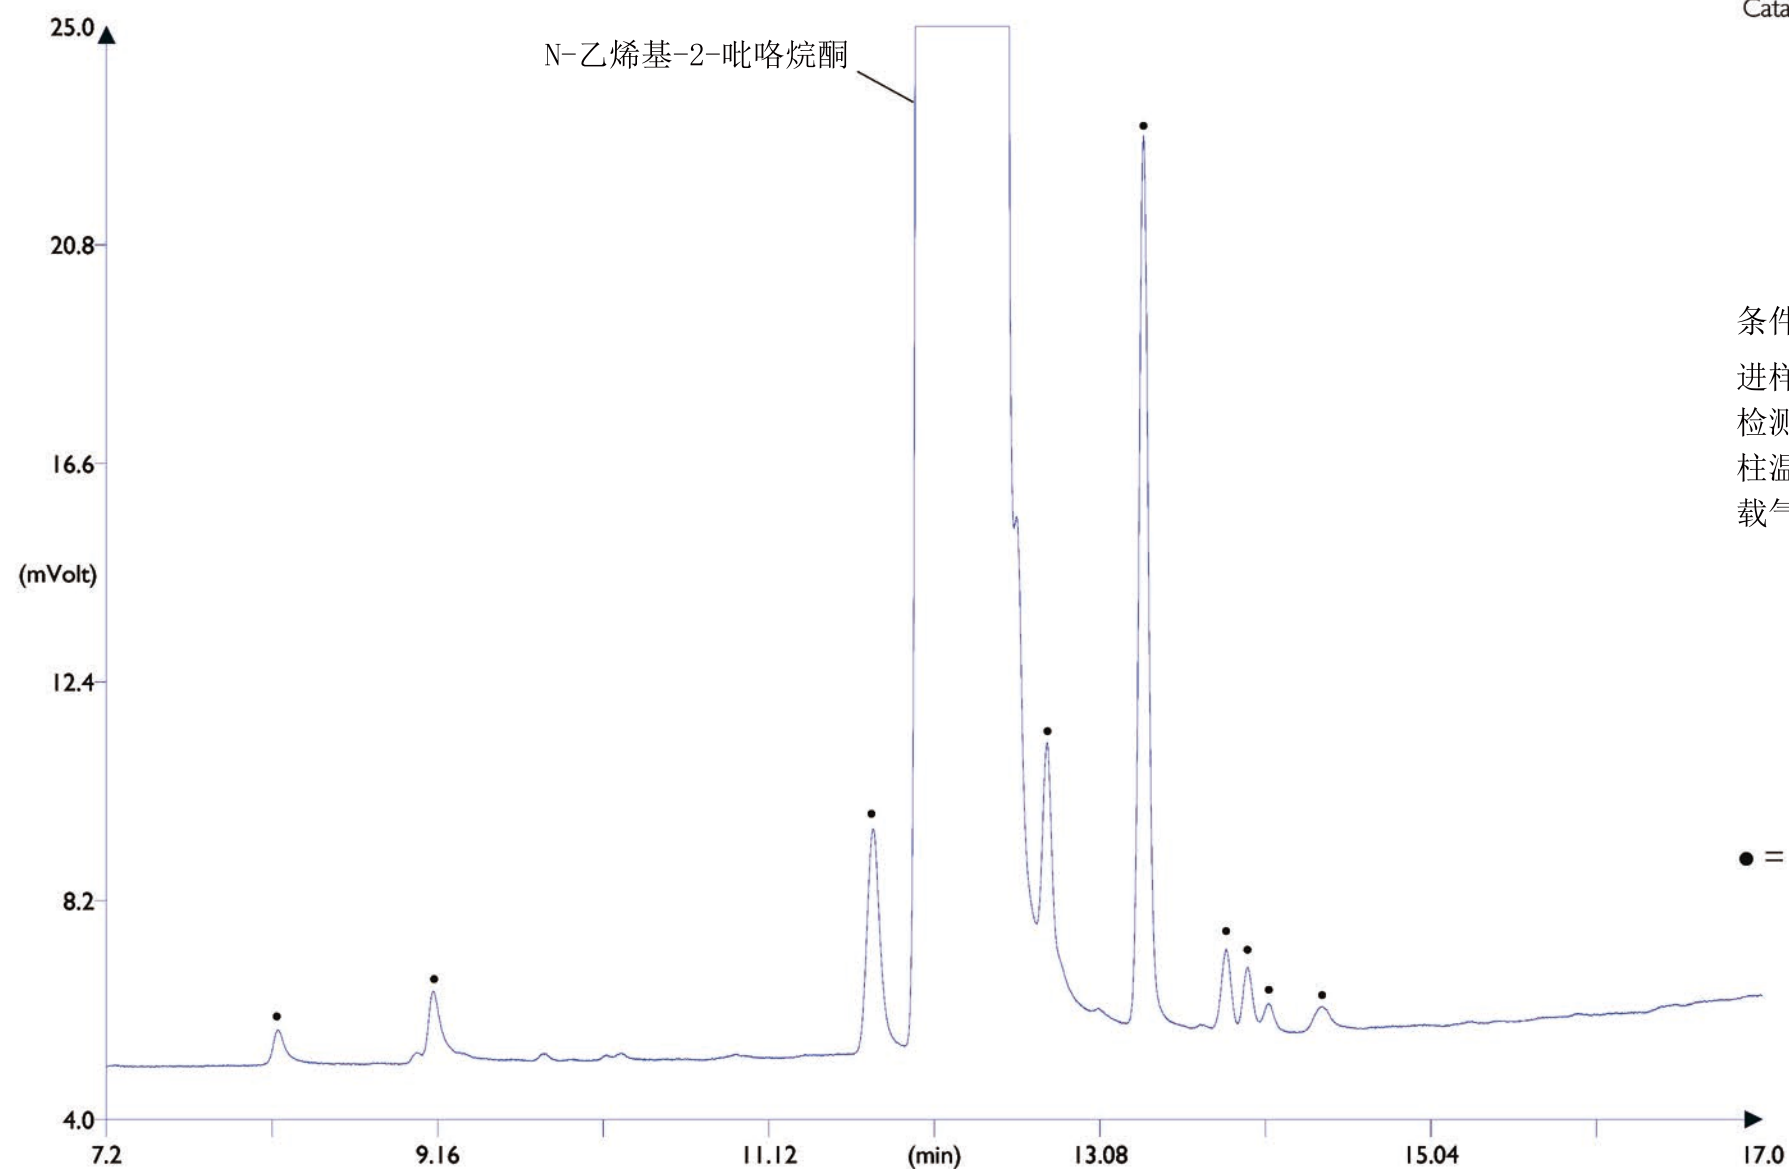

条件:

进样口: 分流 250 $^{\circ}$ C, 50mL/min分流比, 1 μ L进样量

检测器: FID 250 $^{\circ}$ C

柱温箱程序: 40-200 $^{\circ}$ C, 10 $^{\circ}$ C/min

载气: 氦气, 40kPa

● = 杂质